



2 / 32

FIG. 2

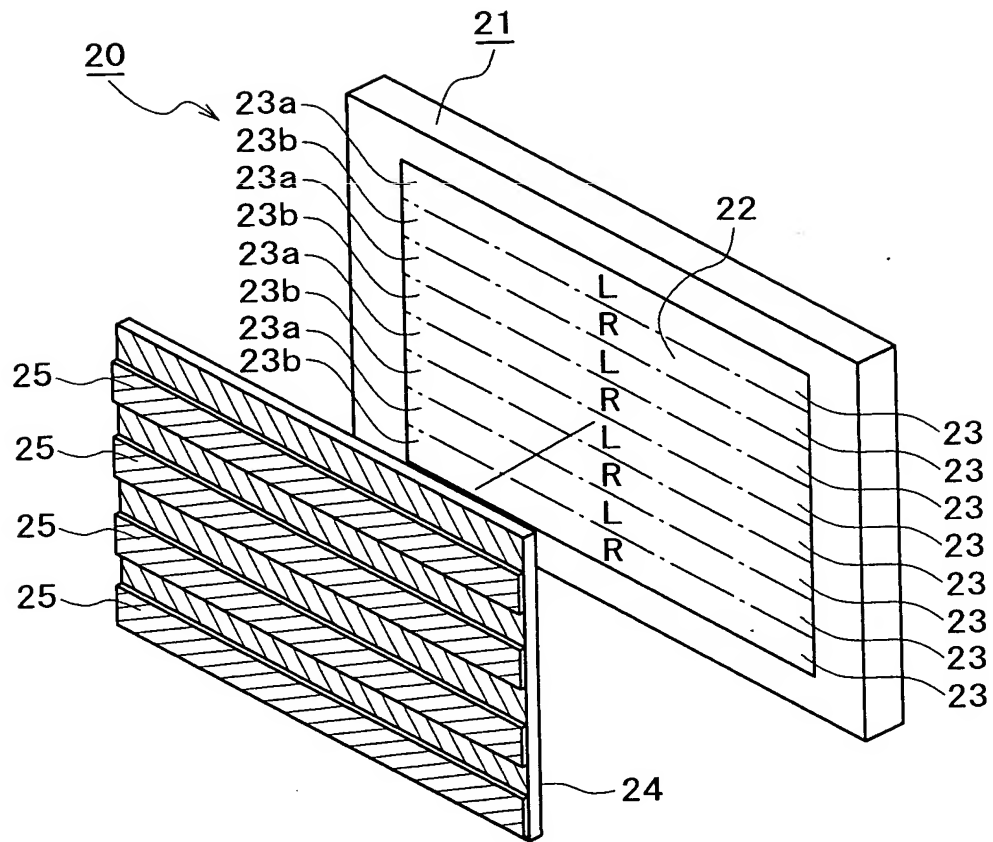


F I G. 3

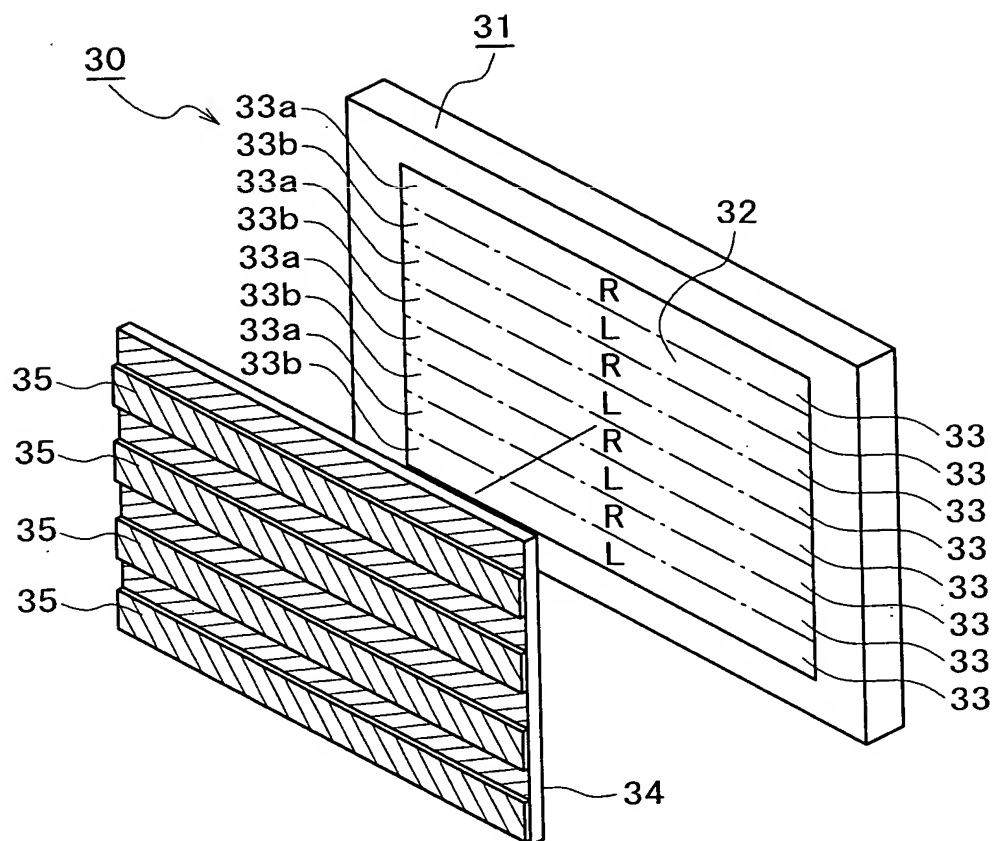


4 / 32

FIG. 4

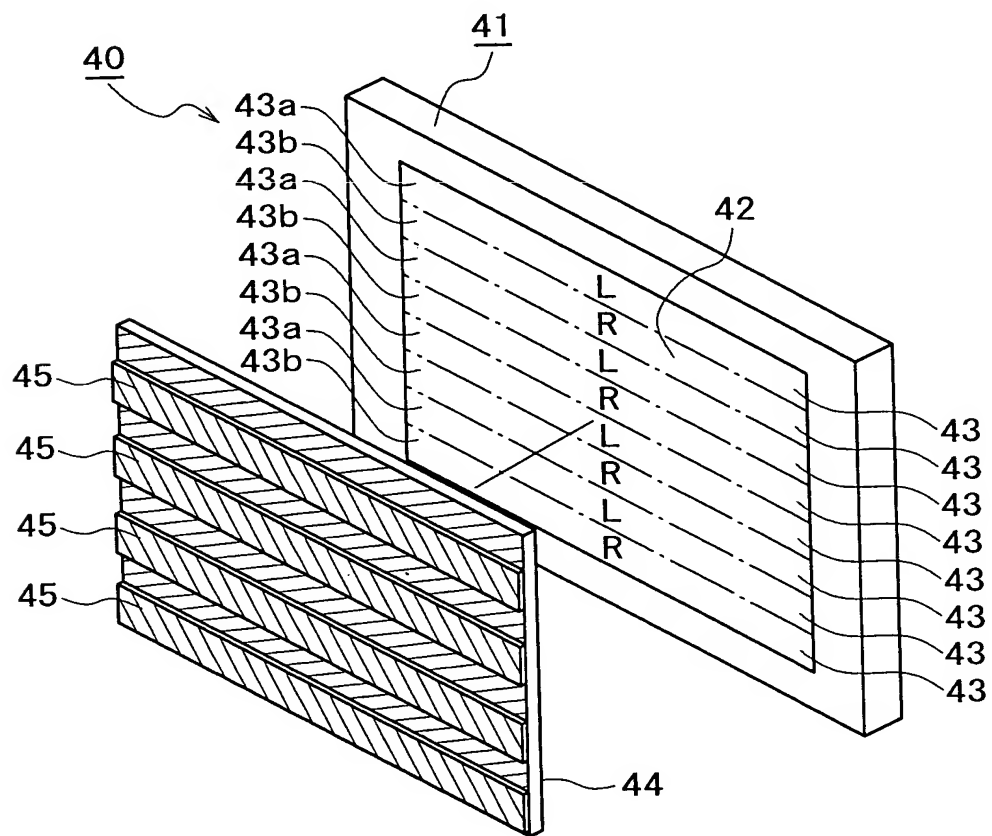


5 / 32

F I G. 5

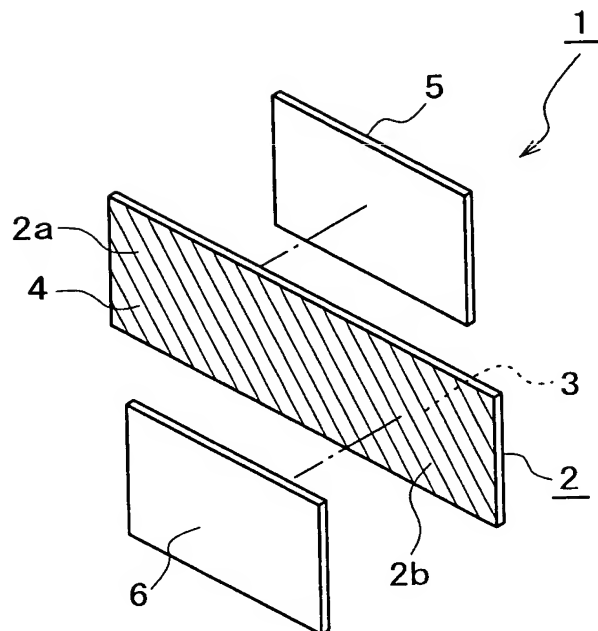


6 / 32

F I G. 6

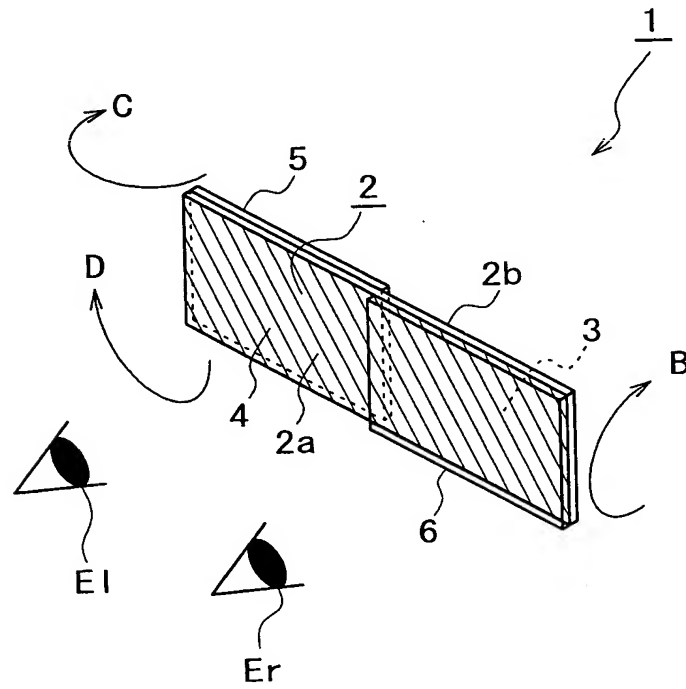


7 / 32

FIG. 7

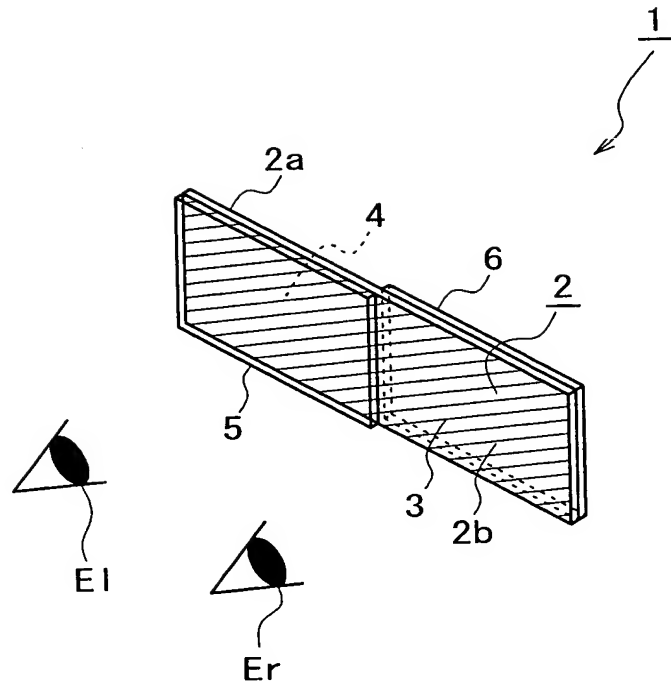

8 / 32

F I G . 8

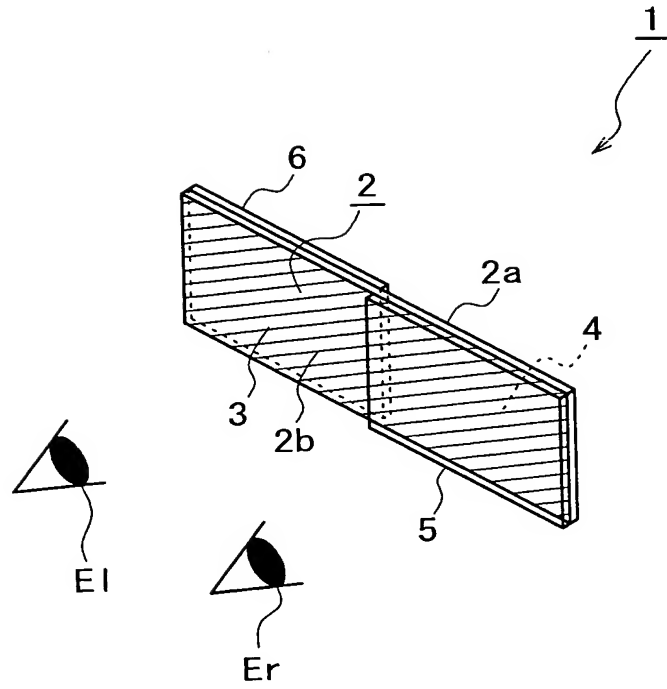

9 / 32

F I G. 9


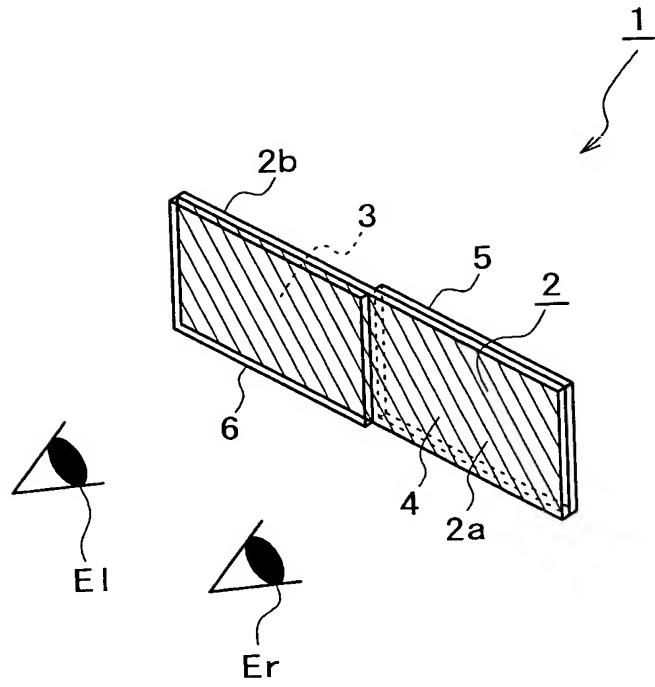


FIG. 10















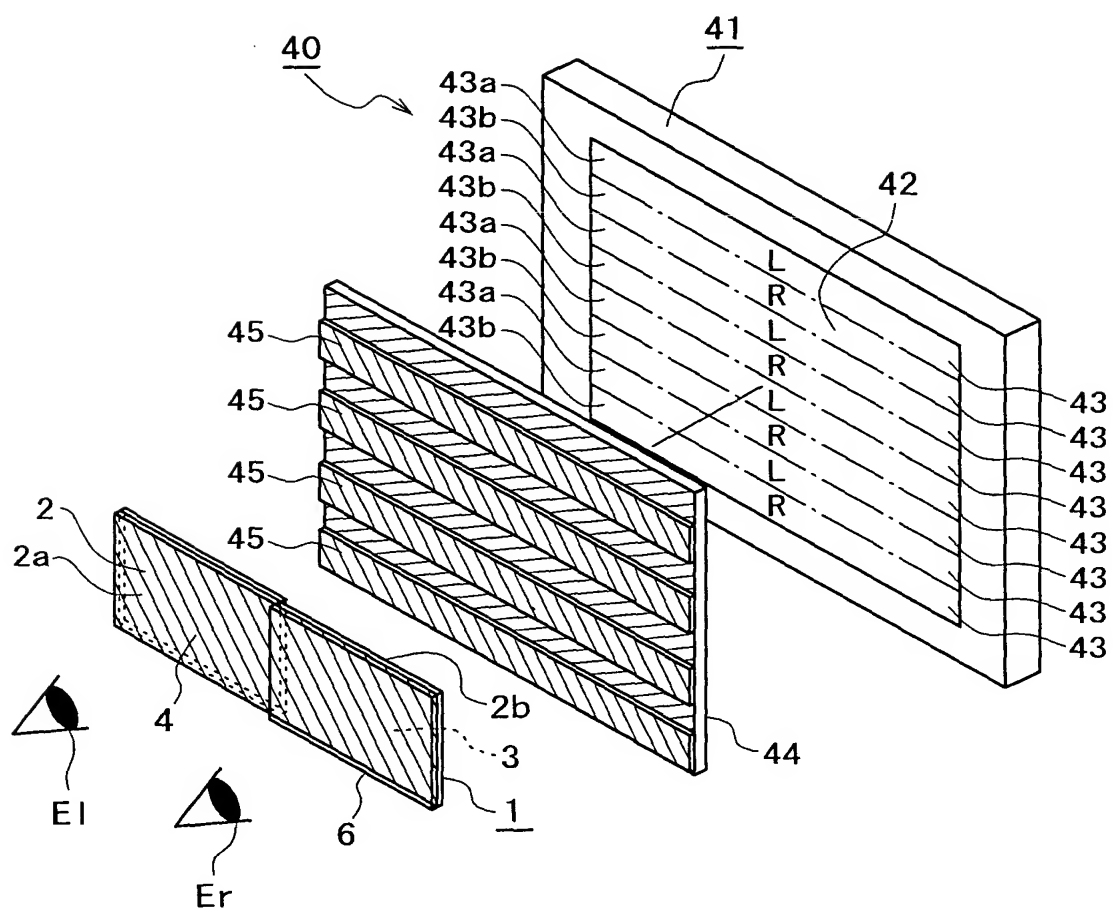











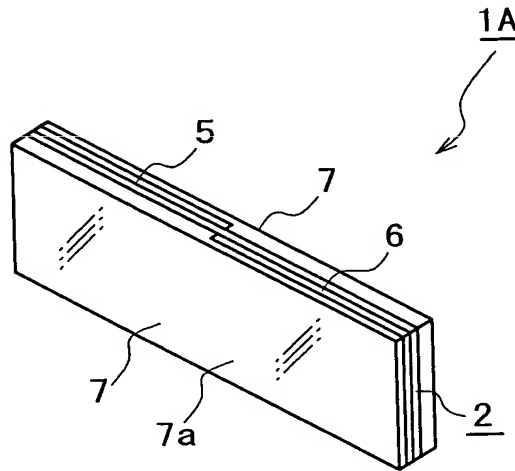
STEREOSCOPIC IMAGE DISPLAY APPARATUS					POLARIZING EYEGLASS DEVICE			
TYPE I	TYPE II	TYPE III	TYPE IV		SERVICE CONDITION A	SERVICE CONDITION B	SERVICE CONDITION C	SERVICE CONDITION D
								
								
								
								
								

FIG. 11


12/32

FIG. 12




13/32

FIG. 13

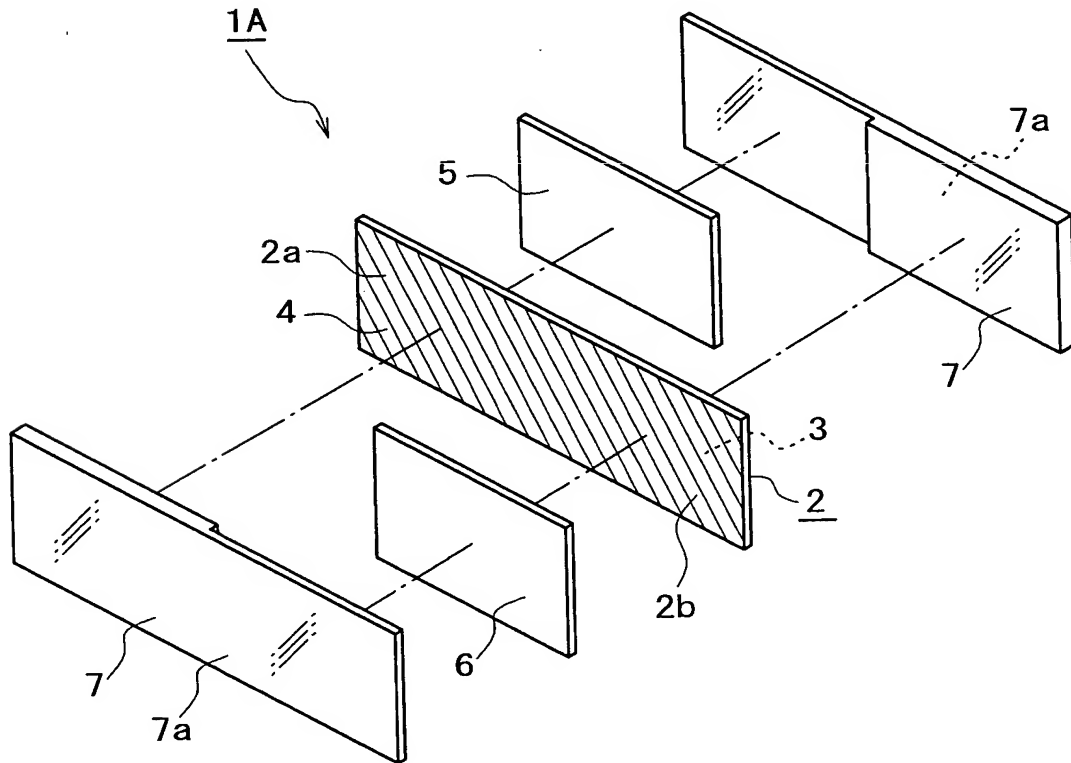


14 / 32

FIG. 14

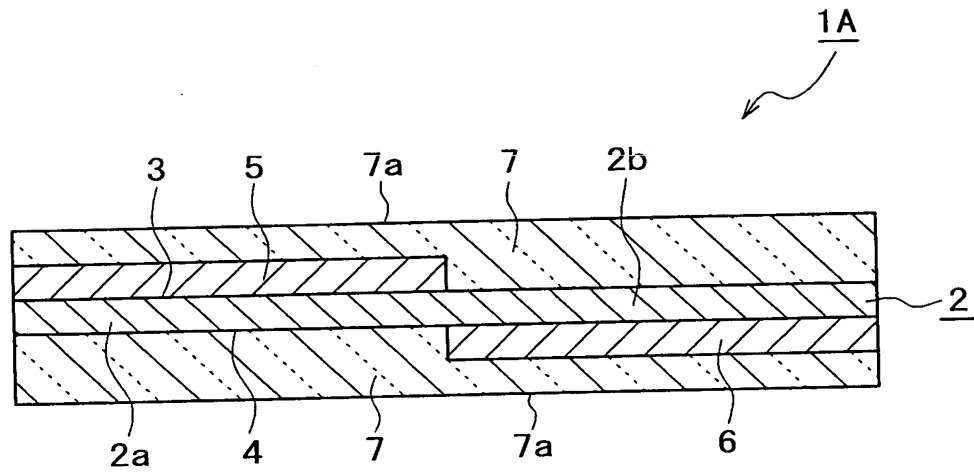

15 / 32

FIG. 15

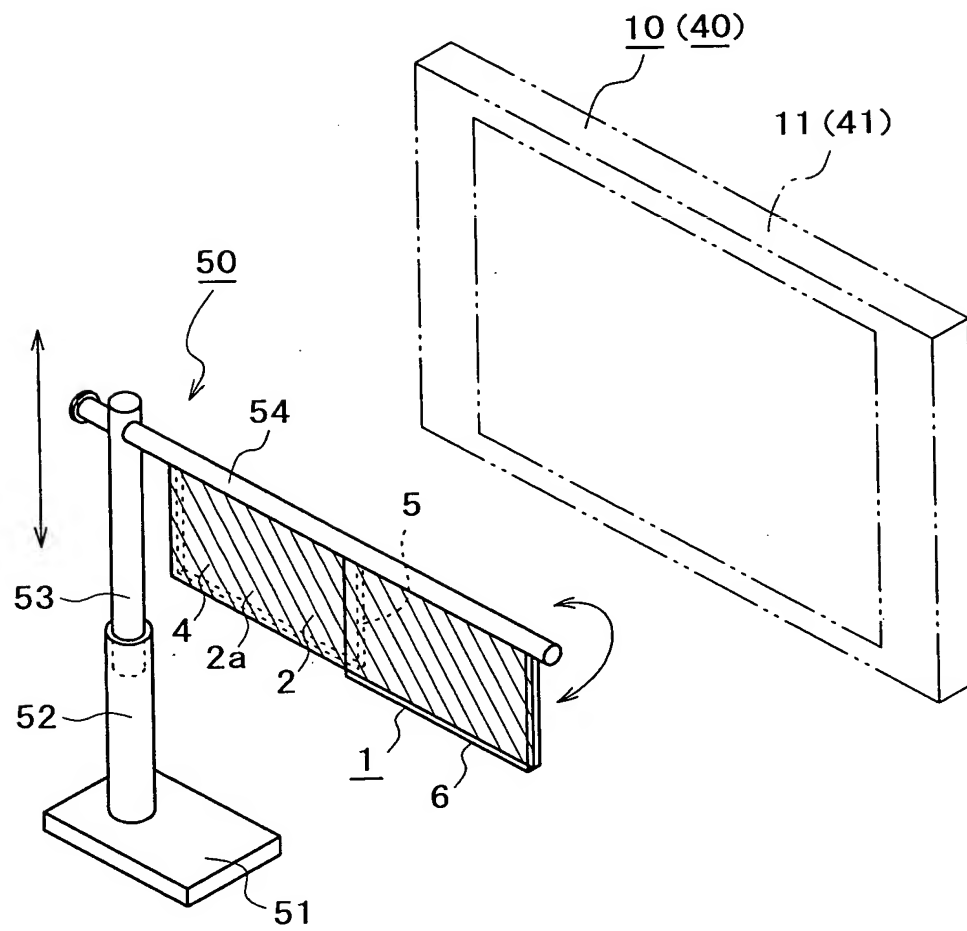

16 / 32

FIG. 16



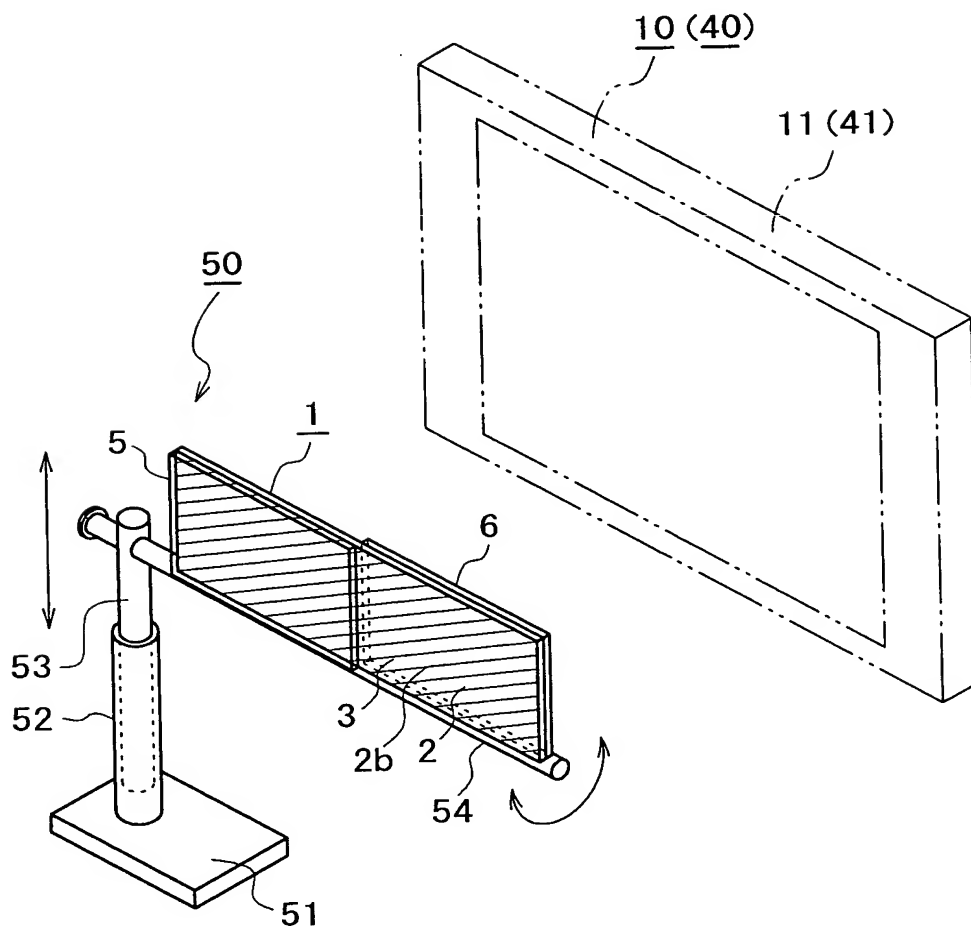


FIG. 17

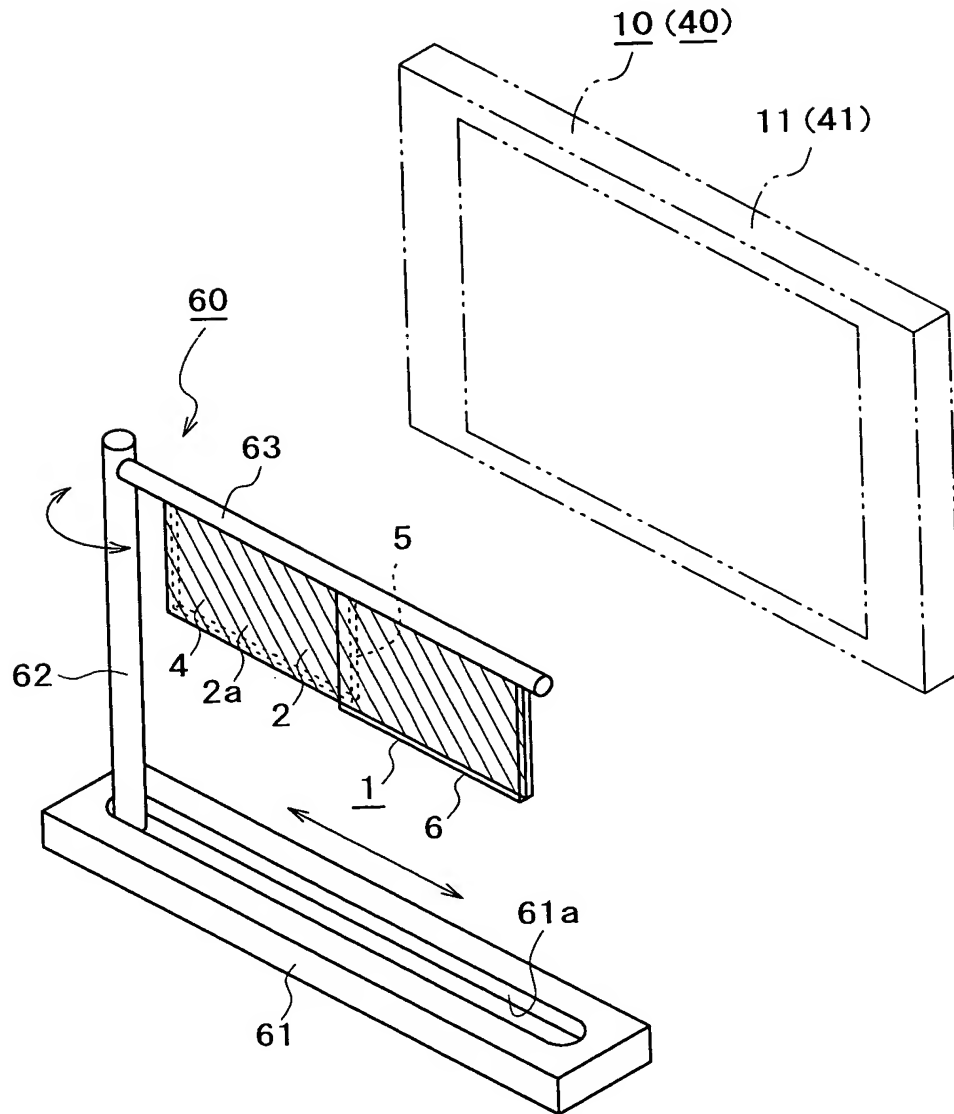


18 / 32

FIG. 18

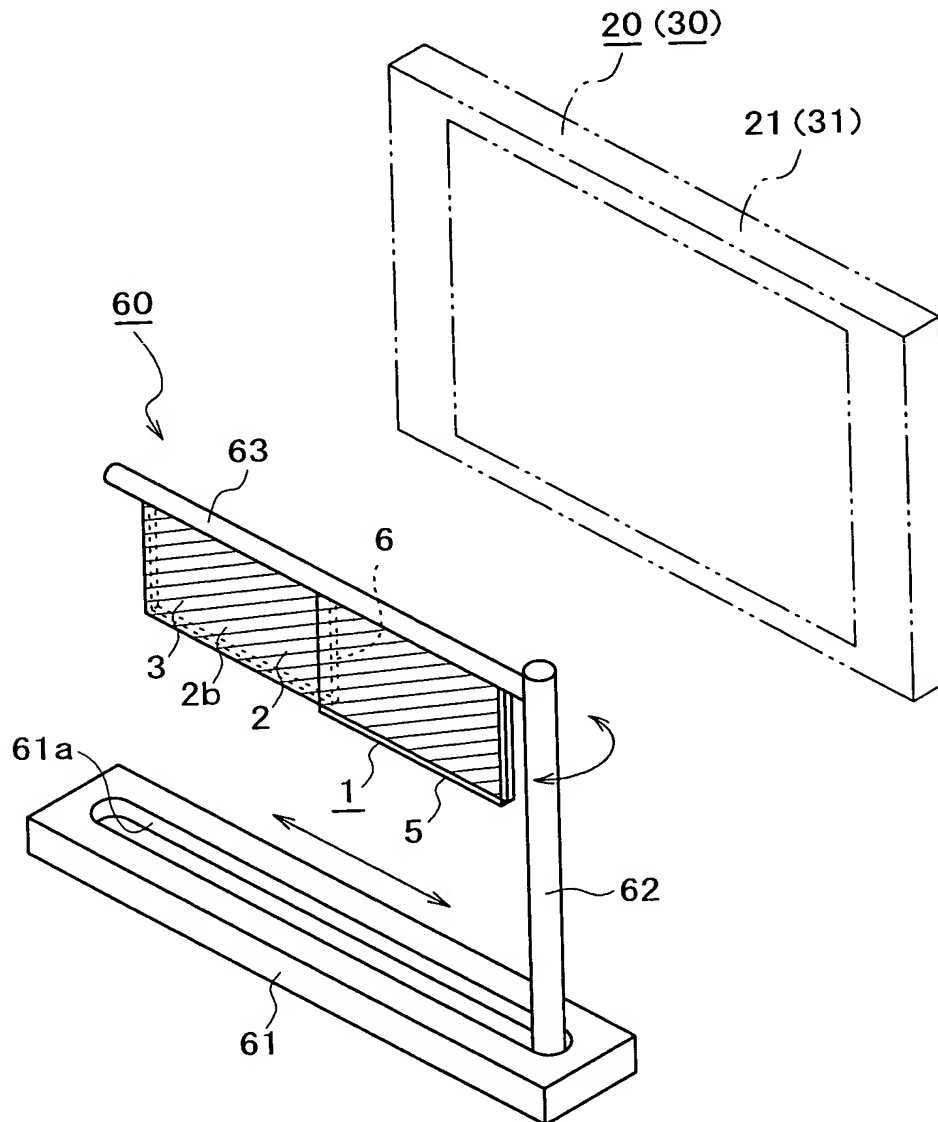


19/32

FIG. 19

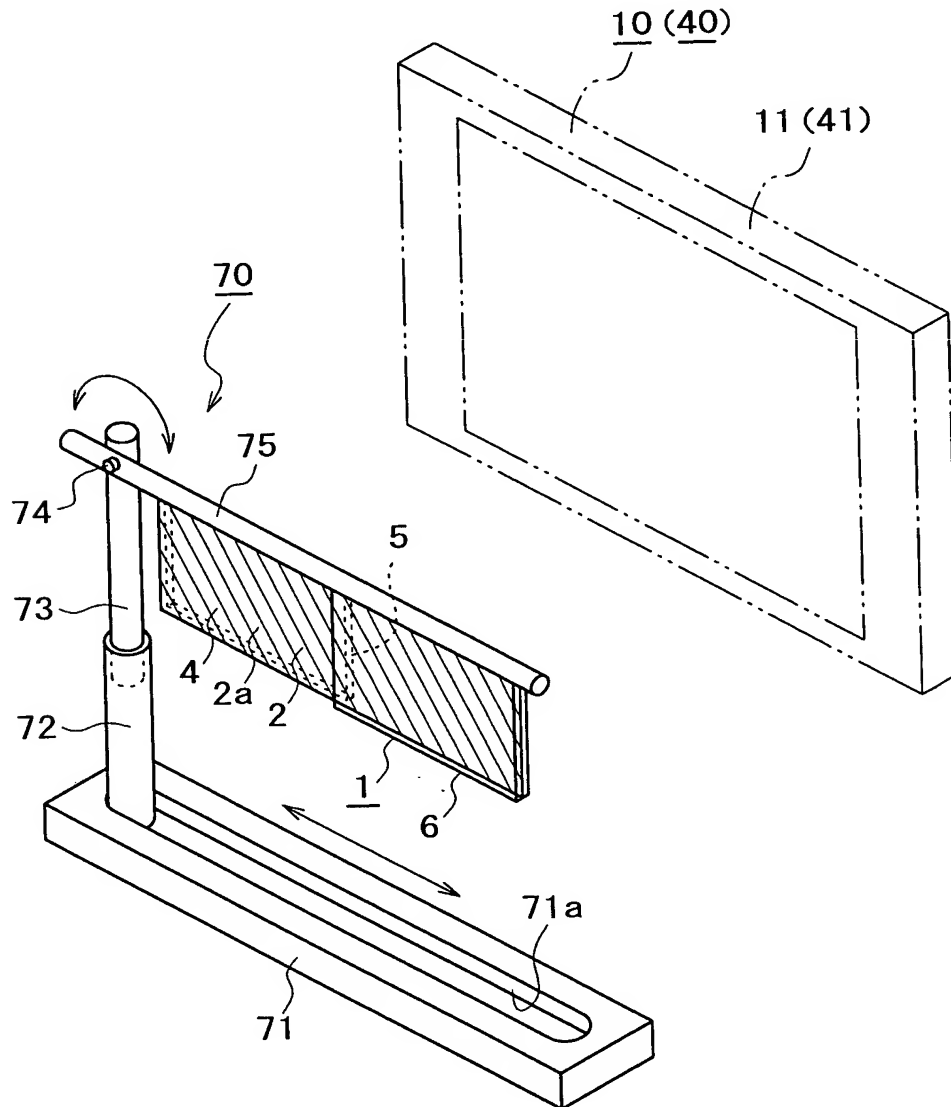


20/32


FIG. 20

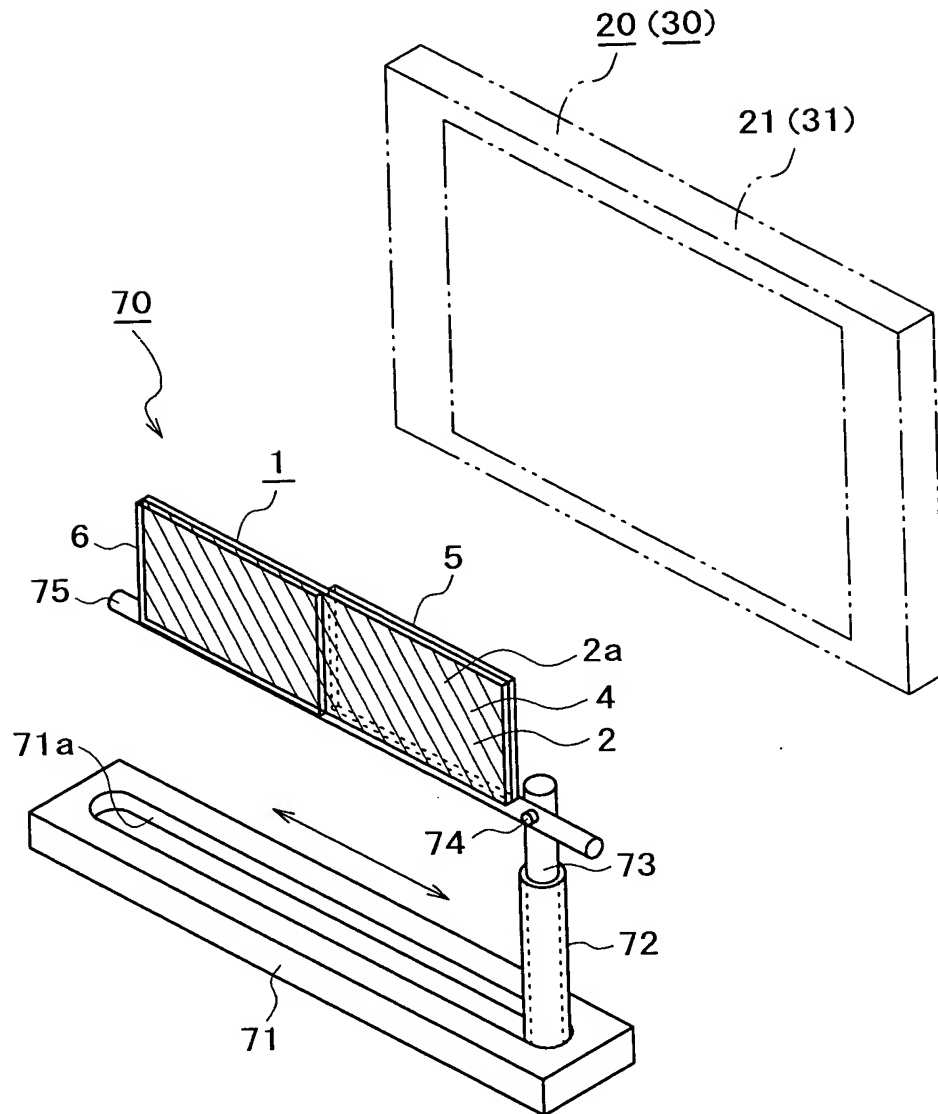

21 / 32


F I G. 2 1

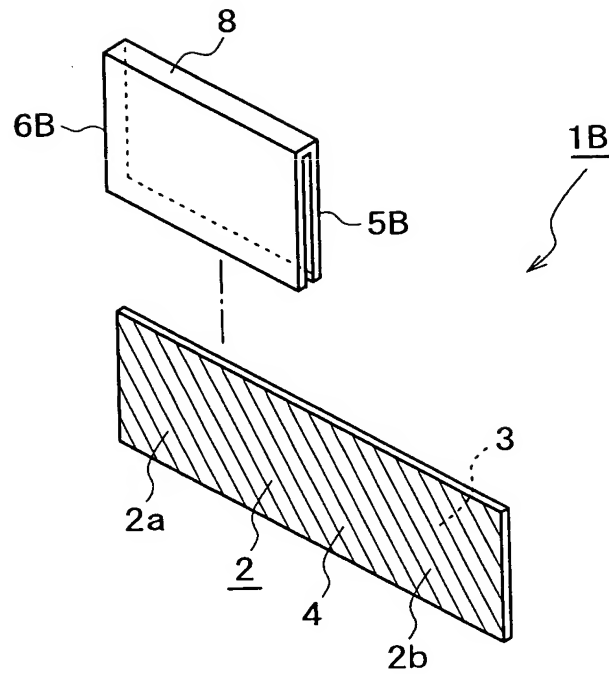

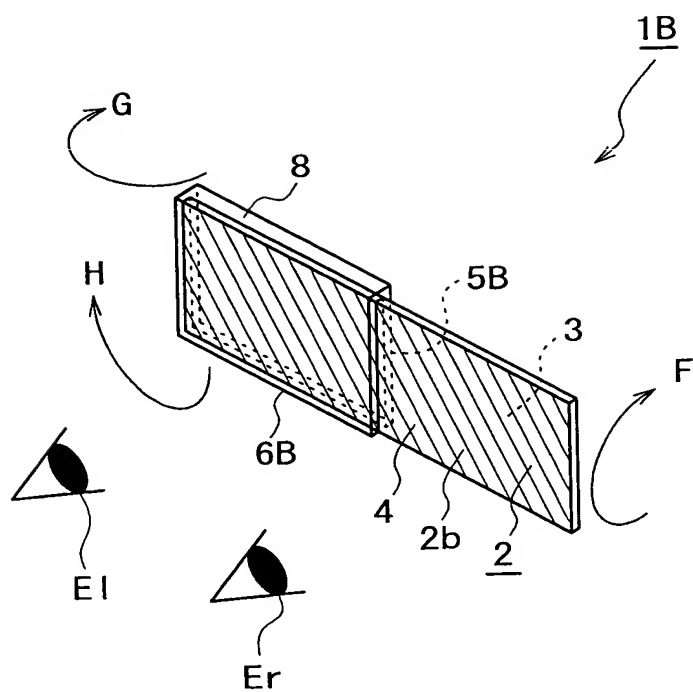


23 / 32

F I G. 2 3

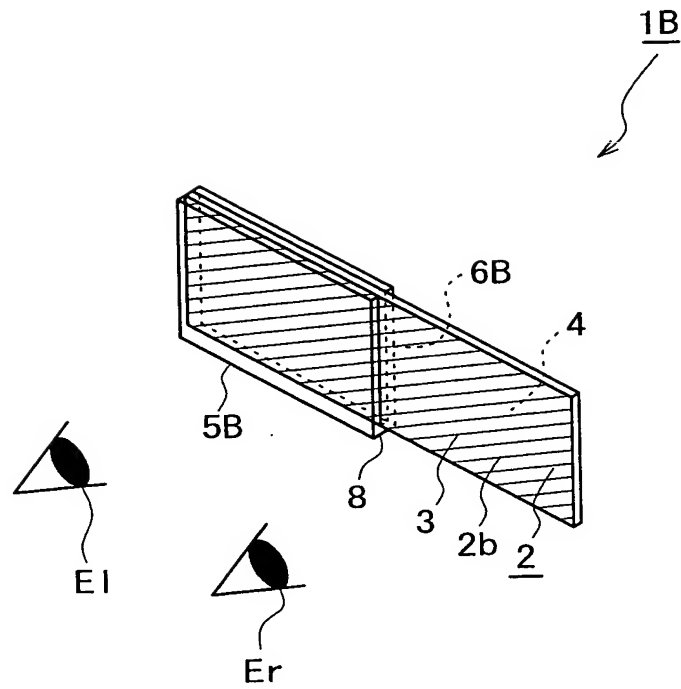


24 / 32


F I G. 2 4

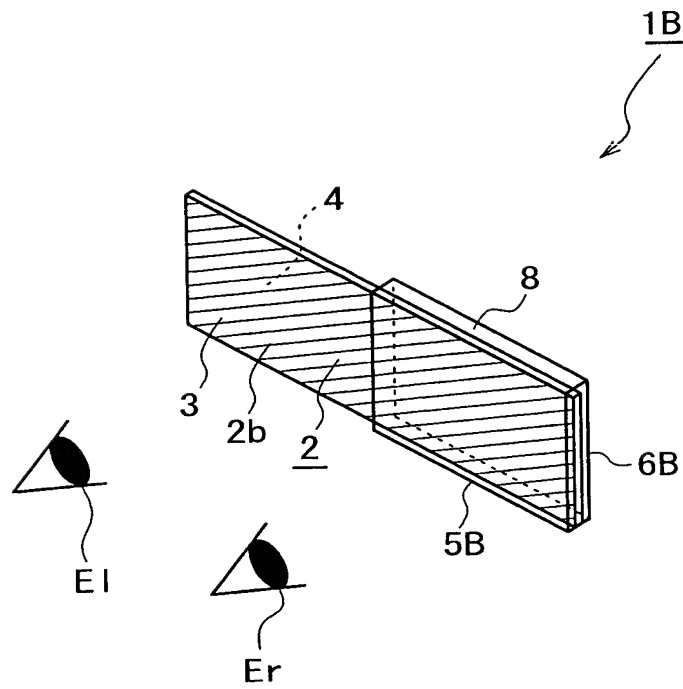

25 / 32

F I G. 2 5

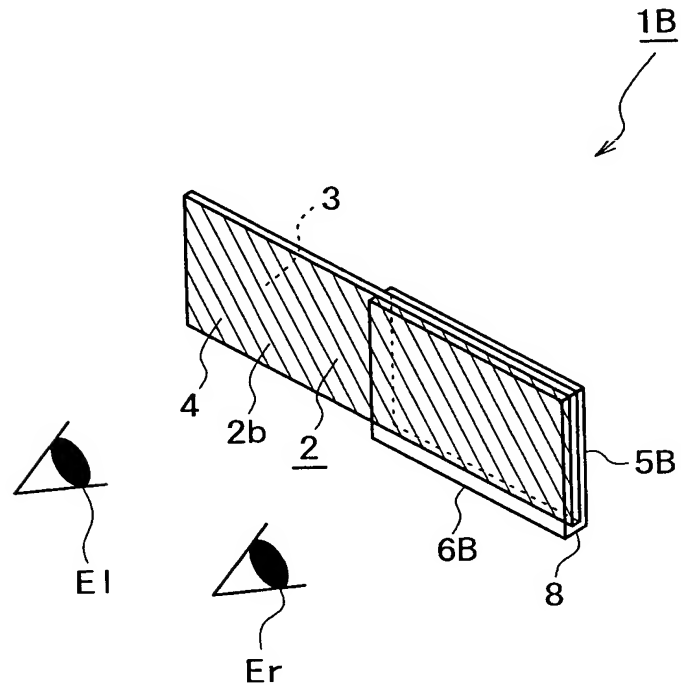

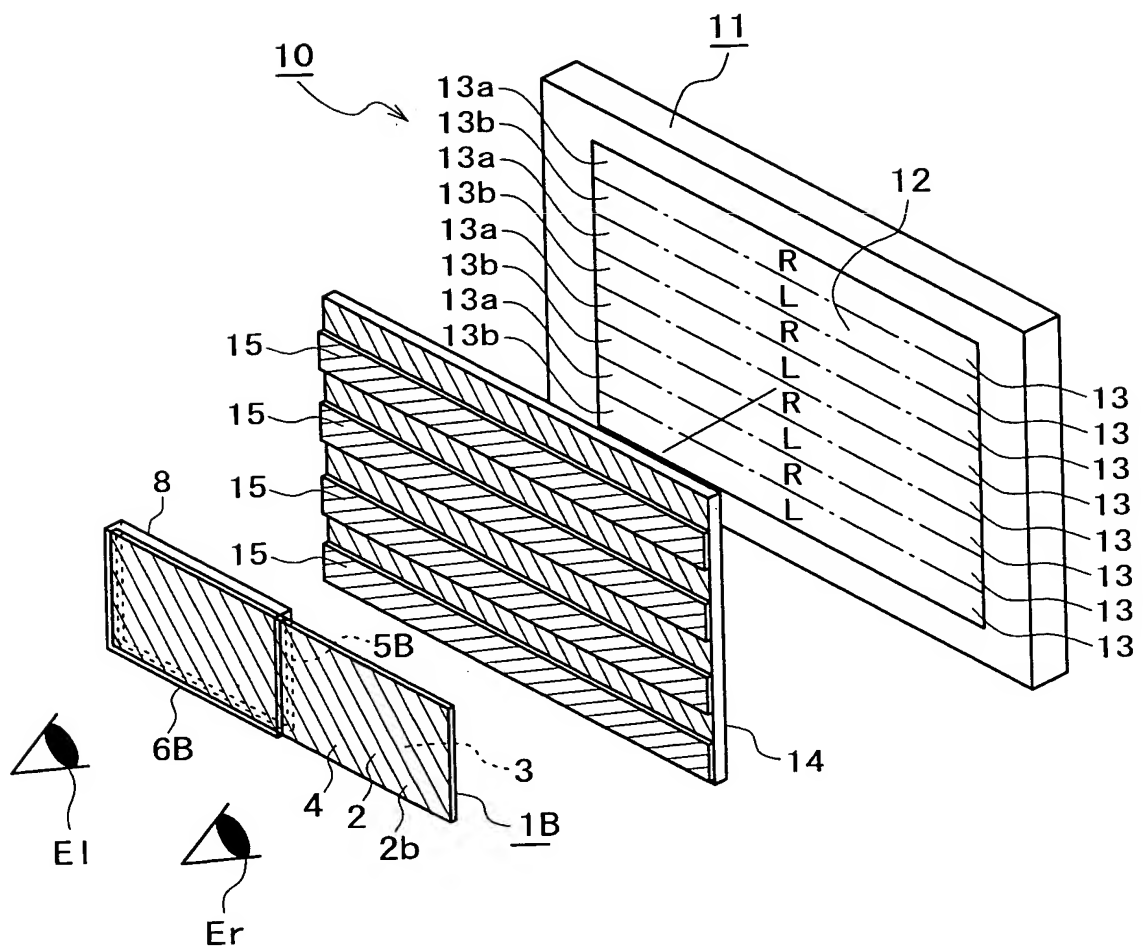









































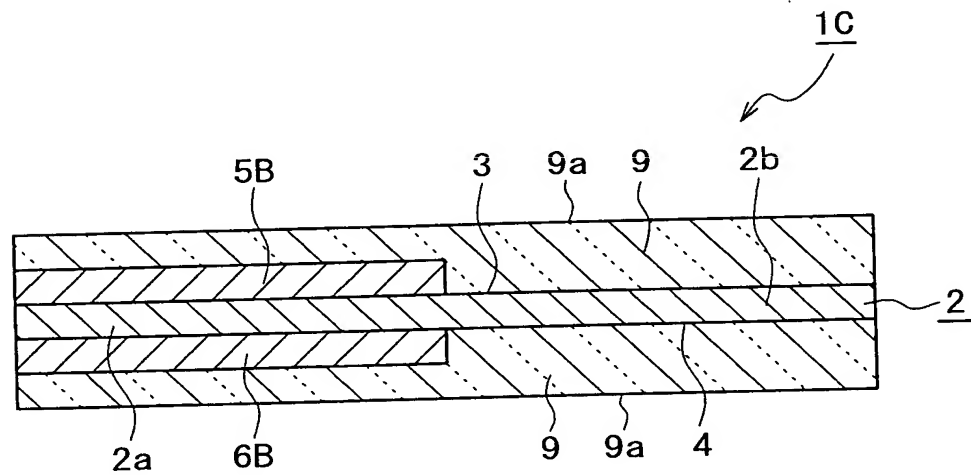
STEREOSCOPIC IMAGE DISPLAY APPARATUS					POLARIZING EYEGLASS DEVICE			
TYPE I	TYPE II	TYPE III	TYPE IV		SERVICE CONDITION E	SERVICE CONDITION F	SERVICE CONDITION G	SERVICE CONDITION H
								
								
								
								
								

FIG. 27


28 / 32

F I G. 2 8




29 / 32

FIG. 29

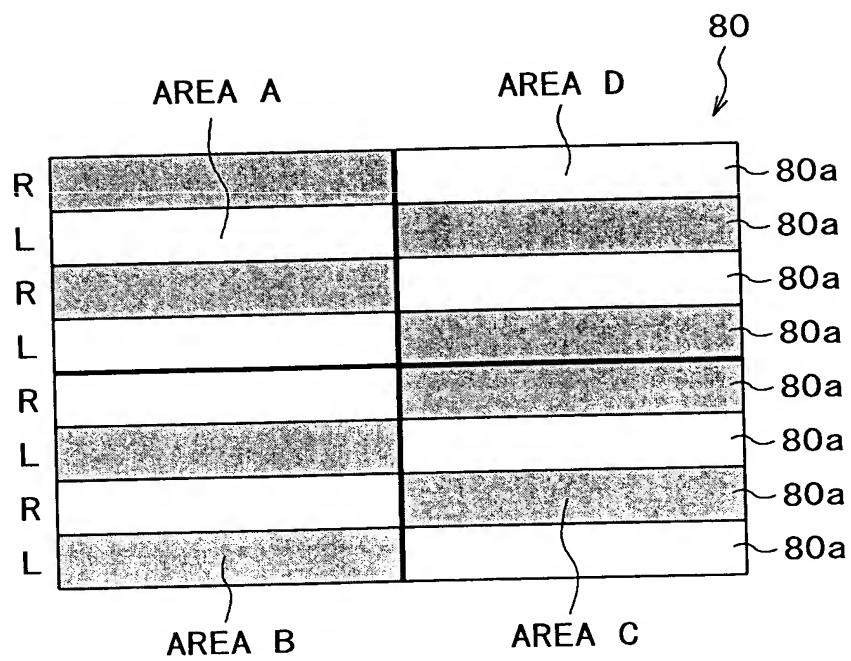


30/32

F I G. 3 0

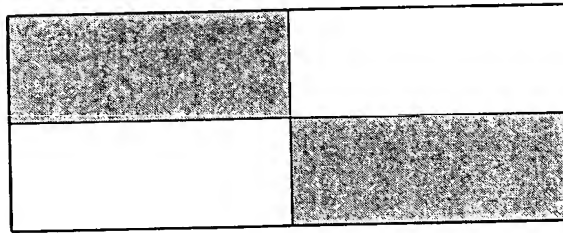


F I G. 3 1

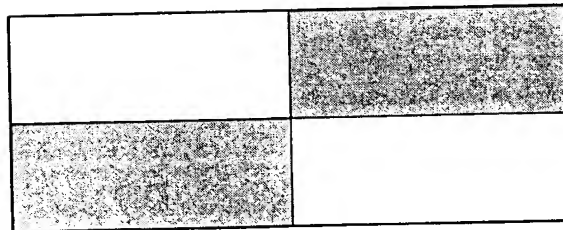

31/32

FIG. 32

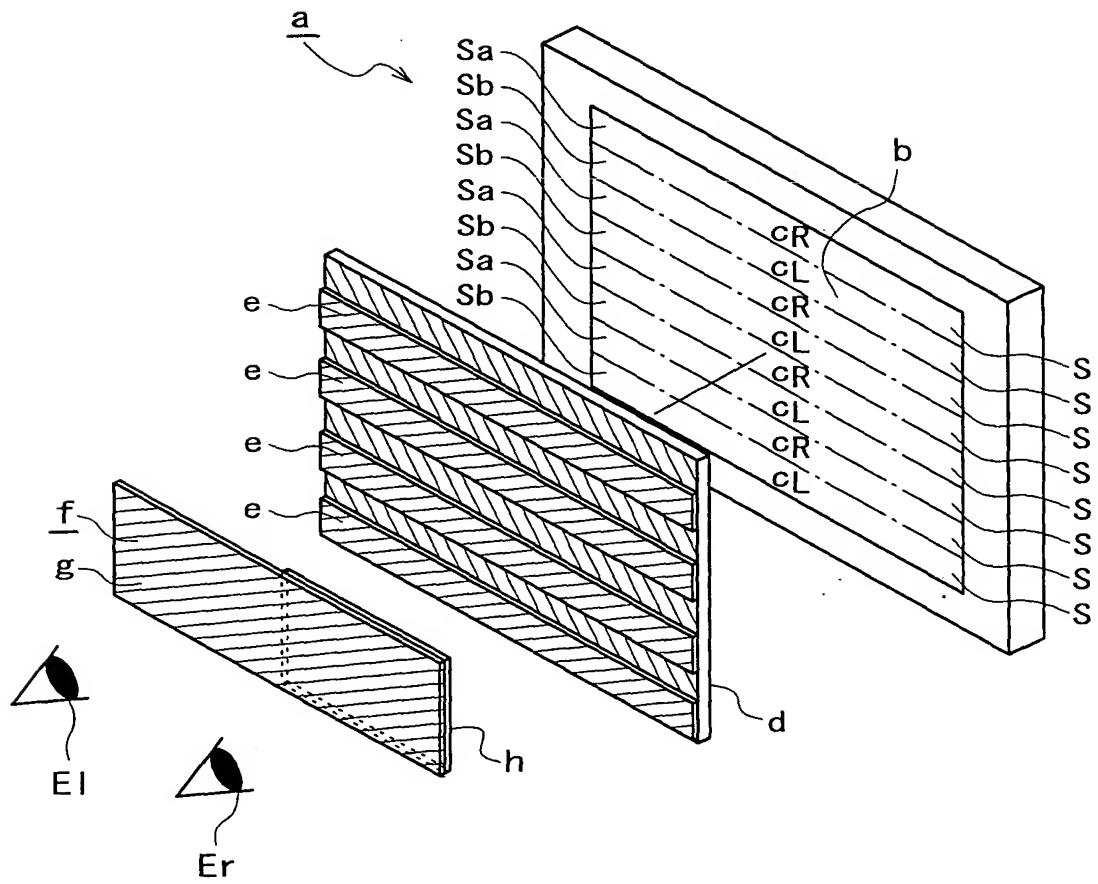

32 / 32

F I G. 3 3

